

2012/13

PI: Dr. Peter Doran  
Compiled by: Hilary Dugan  
*Department of Earth and  
Environmental Sciences  
University of Illinois at Chicago  
845 W. Taylor Street  
hdugan3@uic.edu*

# McMurdo LTER Blue Box Documentation



A guide to sensor installation and programming of LTER limnological stations.  
Updated Dec 17, 2012


# Table of Contents

1. Map .....	3
2. Sensors .....	4
2.1) Available Sensors .....	4
2.2) Programming Information and Manuals.....	5
2.3) Field Setup.....	7
3. Wiring .....	9
3.1) Fryxell, Hoare, ELB Wiring .....	11
3.2) WLB Wiring.....	12
3.3) Lake Miers Wiring.....	12
4. Sensor Changes.....	13
4.1) UNDERWATER PAR sensors. Li-193.....	13
4.2) SURFACE PAR sensors. Li-190.....	13
4.3) Sonar altimeters. Benthos PSA-916 .....	13
4.4) CR1000 Programs.....	13
5. CR1000 Programs .....	15
5.1) Lake Fryxell.....	15
5.2) Lake Hoare .....	19
5.3) East Lake Bonney.....	23
5.4) West Lake Bonney.....	27
5.5) Lake Miers.....	31

# 1. Map



McMurdo Dry Valleys, Antarctica

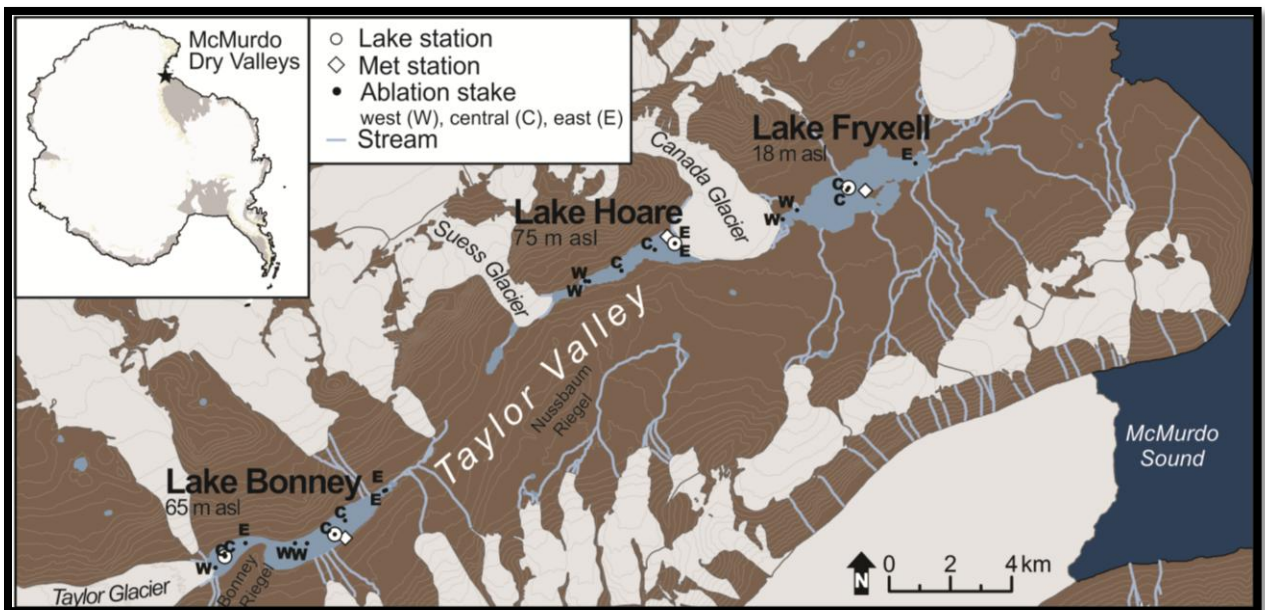

Locations of lake stations in Taylor Valley, Antarctica. Lake Miers not shown.

## 2. Sensors

### 2.1) Available Sensors

SENSORS	SENSOR TYPE	Applications	Company	Units
Surface PAR	LI190 SB Quantum	Measures incident Photosynthetically Active Radiation	LI-COR Biosciences 4421 Superior St. Lincoln, NE 68504 Phone: 800-447-3576 Fax: 402-467-2819	micromoles of quanta per second per square meter ( $\mu\text{mol s}^{-1} \text{m}^{-2}$ )
Underwater PAR	LI-193 Spherical Quantum Sensor	Measures PAR coming from all directions.	LI-COR Biosciences 4421 Superior St. Lincoln, NE 68504 Phone: 800-447-3576 Fax: 402-467-2819	
Ablation Transducer (pressure transducer)	CS455 (at LF, LH, ELB) and Druck Pressure Transducer PDCR 1830 (at WLB and Miers)	Continuous lake ice ablation measurement	Campbell Sci. Logan, UT	m
Lake Level (Stage) Transducer	CS455 (at LF, LH, ELB) and Druck Pressure Transducer PDCR (at WLB)	Continuous lake level measurements	Campbell Sci. Logan, UT	m
Water Temperature	CS455 (at LF, LH, ELB) and Druck Pressure Transducer PDCR (at WLB)	Continuous water temperature measurements	Campbell Sci. Logan, UT	$^{\circ}\text{C}$
Ice Thickness	Benthos PSA-916 Sonar Altimeter	Narrow beam acoustic signal	Benthos, Inc. 49 Edgerton Drive North Falmouth, MA 02556	m
Surface Temperature	Campbell Scientific CS107	Surface temperature	Campbell Sci. Logan, UT	$^{\circ}\text{C}$

## 2.2) Programming Information and Manuals

### (1) LI190 SB Quantum



Sensor details:

[http://www.licor.com/env/Products/Sensors/190/li190\\_description.jsp](http://www.licor.com/env/Products/Sensors/190/li190_description.jsp)

**Instruction Manual from Campbell Scientific:**

<http://www.campbellsci.com/documents/manuals/li190sb.pdf>

### (2) LI-193 Spherical Quantum Sensor



Sensor details:

[http://www.licor.com/env/Products/Sensors/193UW/li193\\_description.jsp](http://www.licor.com/env/Products/Sensors/193UW/li193_description.jsp)

[http://www.licor.com/env/PDF\\_Files/193SA.pdf](http://www.licor.com/env/PDF_Files/193SA.pdf)

### (3) Druck Pressure Transducer (WLB and Lake Miers only)



Sensor details:

<http://www.gesensing.com/products/resources/datasheets/PDSA065june02.pdf>

**Instruction Manual from Campbell Scientific**

<http://www.campbellsci.com/documents/manuals/cs420-1.pdf>

**Note:** Ablation Transducer (frequently called Pressure Transducer) and Lake Level Transducer (also known as Stage Transducer) are both the same type of transducers. The only difference between two is that they are differently programmed – one for measuring the Ice ablation and the other for measuring the lake level.

### (4) CS455 Pressure Transducer (LF, LH, ELB,WLB)



**Instruction Manual from Campbell Scientific**

<http://s.campbellsci.com/documents/us/manuals/cs450-cs455.pdf>

**(5) CR1000 DataLogger**



**Measurements and Control Module Operator's Manual**  
<http://s.campbellsci.com/documents/us/manuals/cr1000.pdf>

**(6) Benthos PSA-916 Sonar Altimeter**




**Sensor Manual**  
[www.benthos.com/pdf/PSA900\\_916.pdf](http://www.benthos.com/pdf/PSA900_916.pdf)

**(6) CS107 Temperature Sensor**



**Sensor Manual**  
<http://s.campbellsci.com/documents/us/manuals/107.pdf>

### 2.3) Field Setup

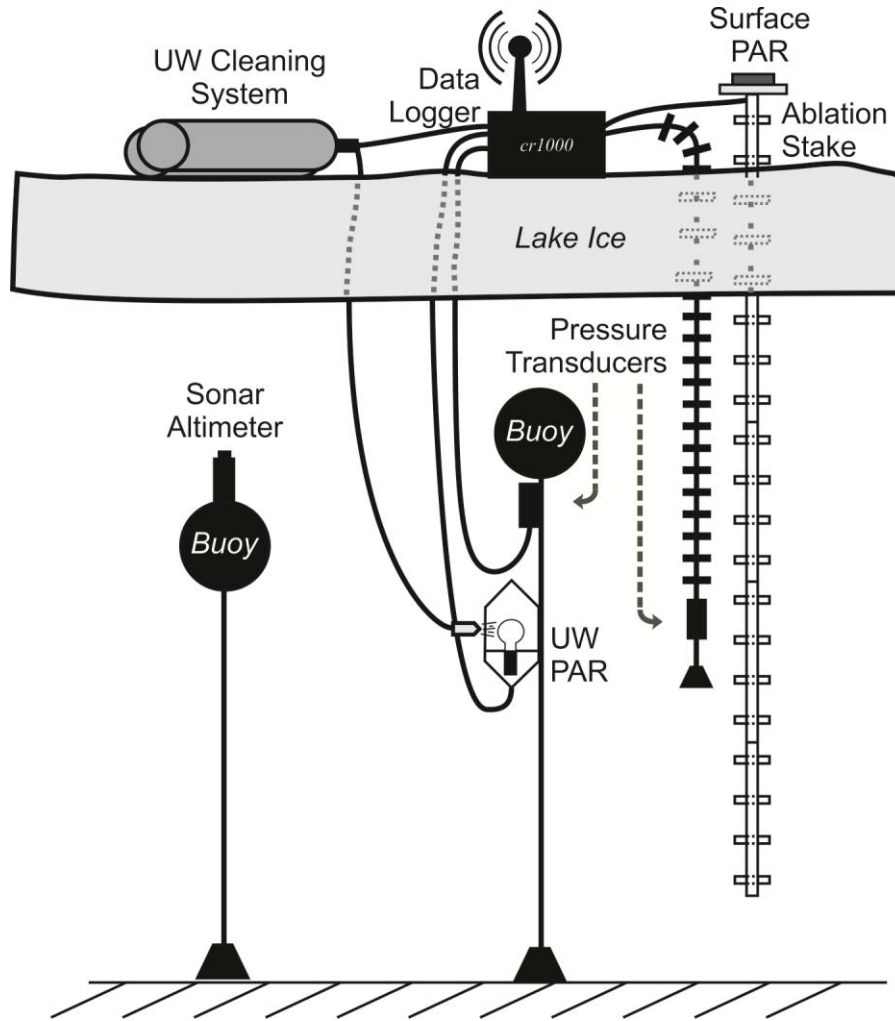

**Figure 1. Setup of datalogger and sensors housed on the ice surface of each lake. The moored and hanging pressure transducers are used to calculate changes in stage and surface ice ablation. Note: Lake Miers does not have a sonar altimeter or UW cleaning system.**

UW PAR is fixed to the buoy. However, due to continuous lake level change, depth corrections are necessary for UW PAR data. Deployment depths are measured from piezometric water level:

- Lake Fryxell: 8 m
- Lake Hoare: 10.1 m
- ELB: 10.06 m
- WLB: 9.86 m
- Lake Miers: 9.90 m

As of 2012/13.

Year round telemetry has been installed at all lakes.


UW PAR cleaning system has been installed at Fryxell, Hoare, ELB, and WLB.

Surface temperature sensors/sonar altimeters installed at Fryxell, Hoare, ELB, and WLB.


Two 88Ah 12V batteries installed at each blue box.

A second set of UW PAR sensors has been added hanging from the ice.

**Blue box at West Lobe Bonney.**  
**Outriggers are facing main wind direction to prevent box from flipping.**

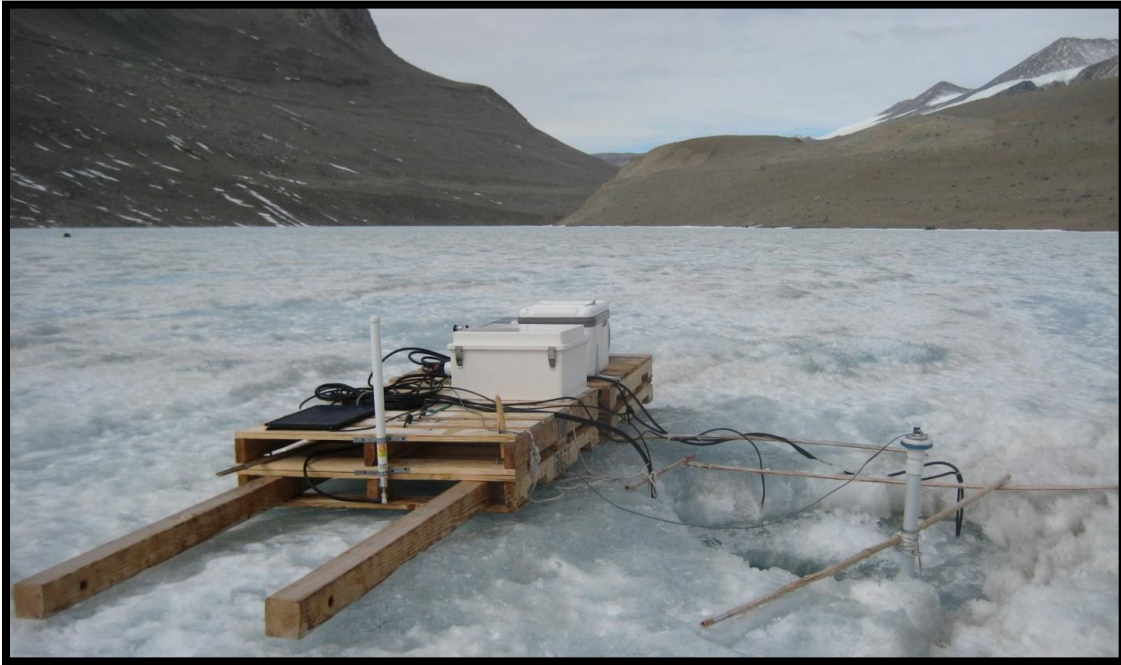


**Blue box surface instrumentation**

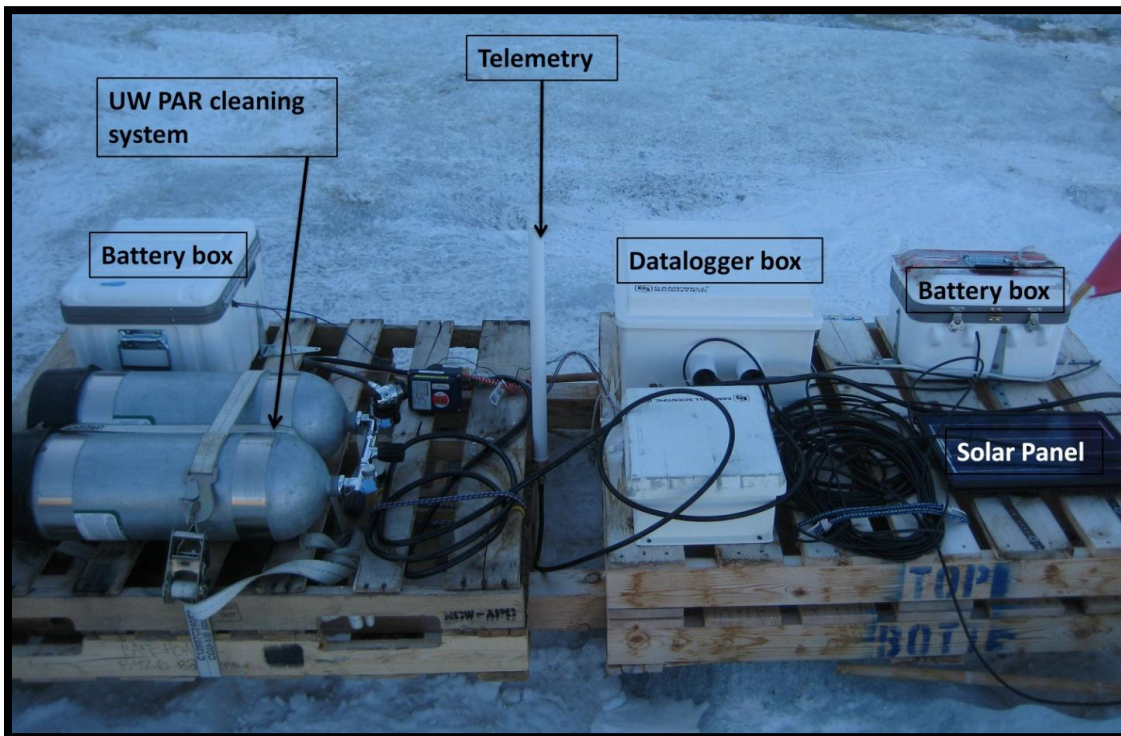




### 3. Wiring

Wiring panel at Lake Fryxell.

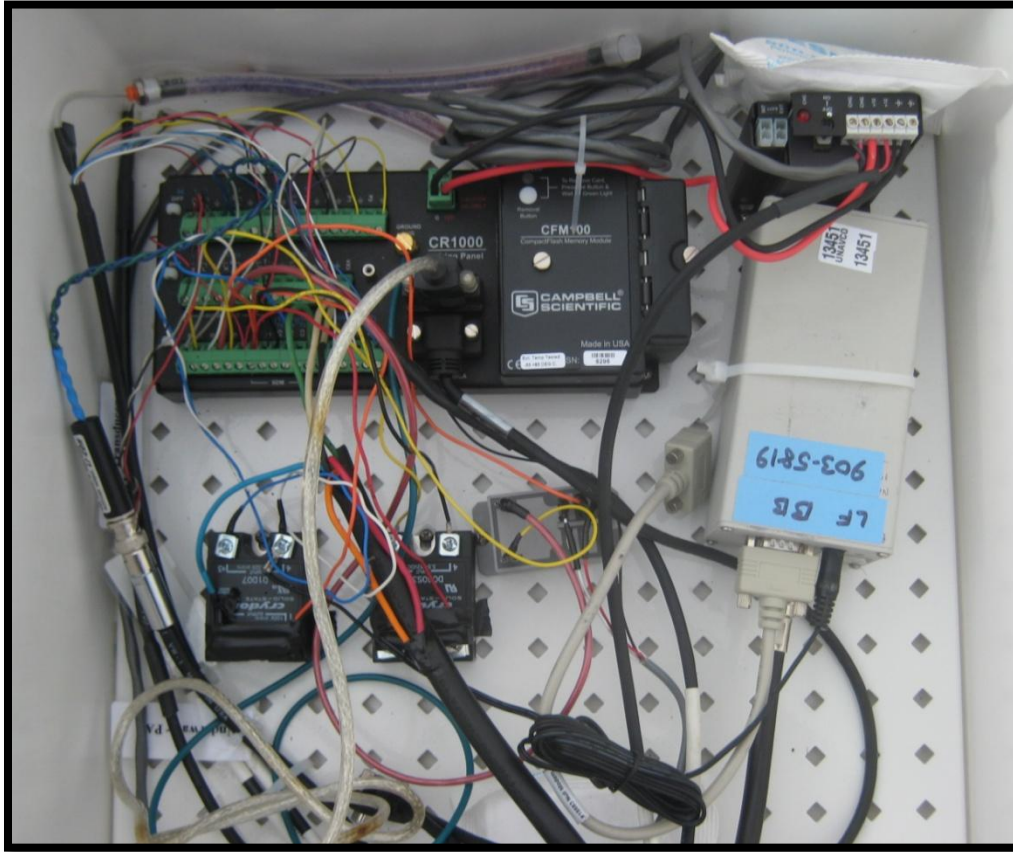


Relays at Lake Fryxell. Two Crydom D1D07 relays for sonar altimeter and telemetry, SPDT relay for underwater cleaning system.

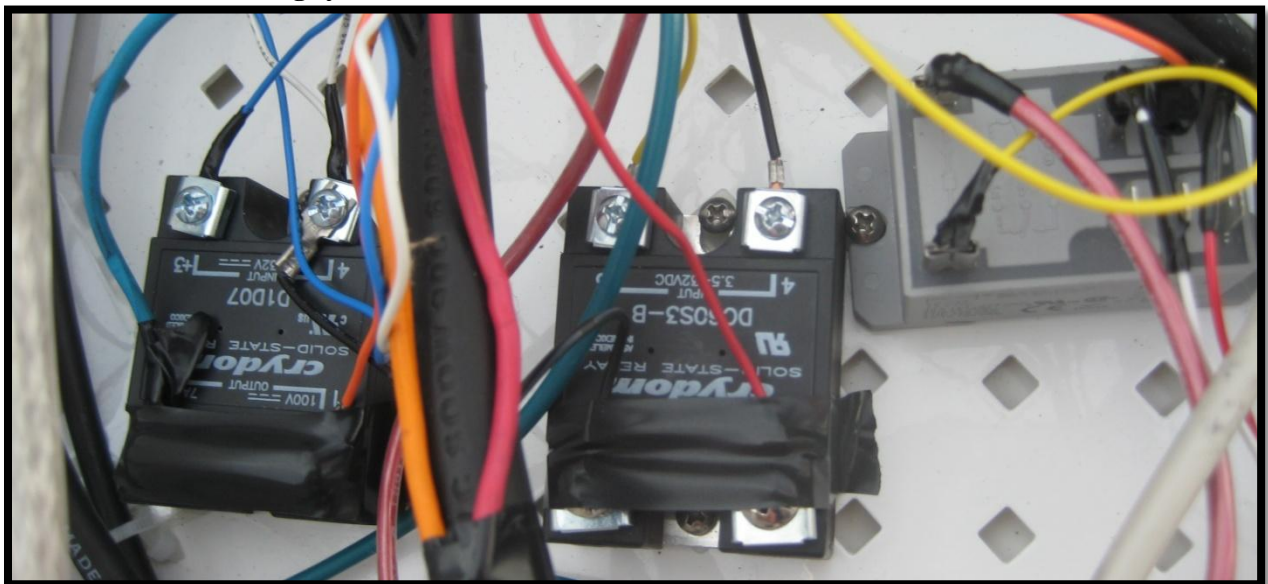

# Cr1000 Wiring Diagram for TV Blue Boxes

by: Hilary Dugan Sep 2012

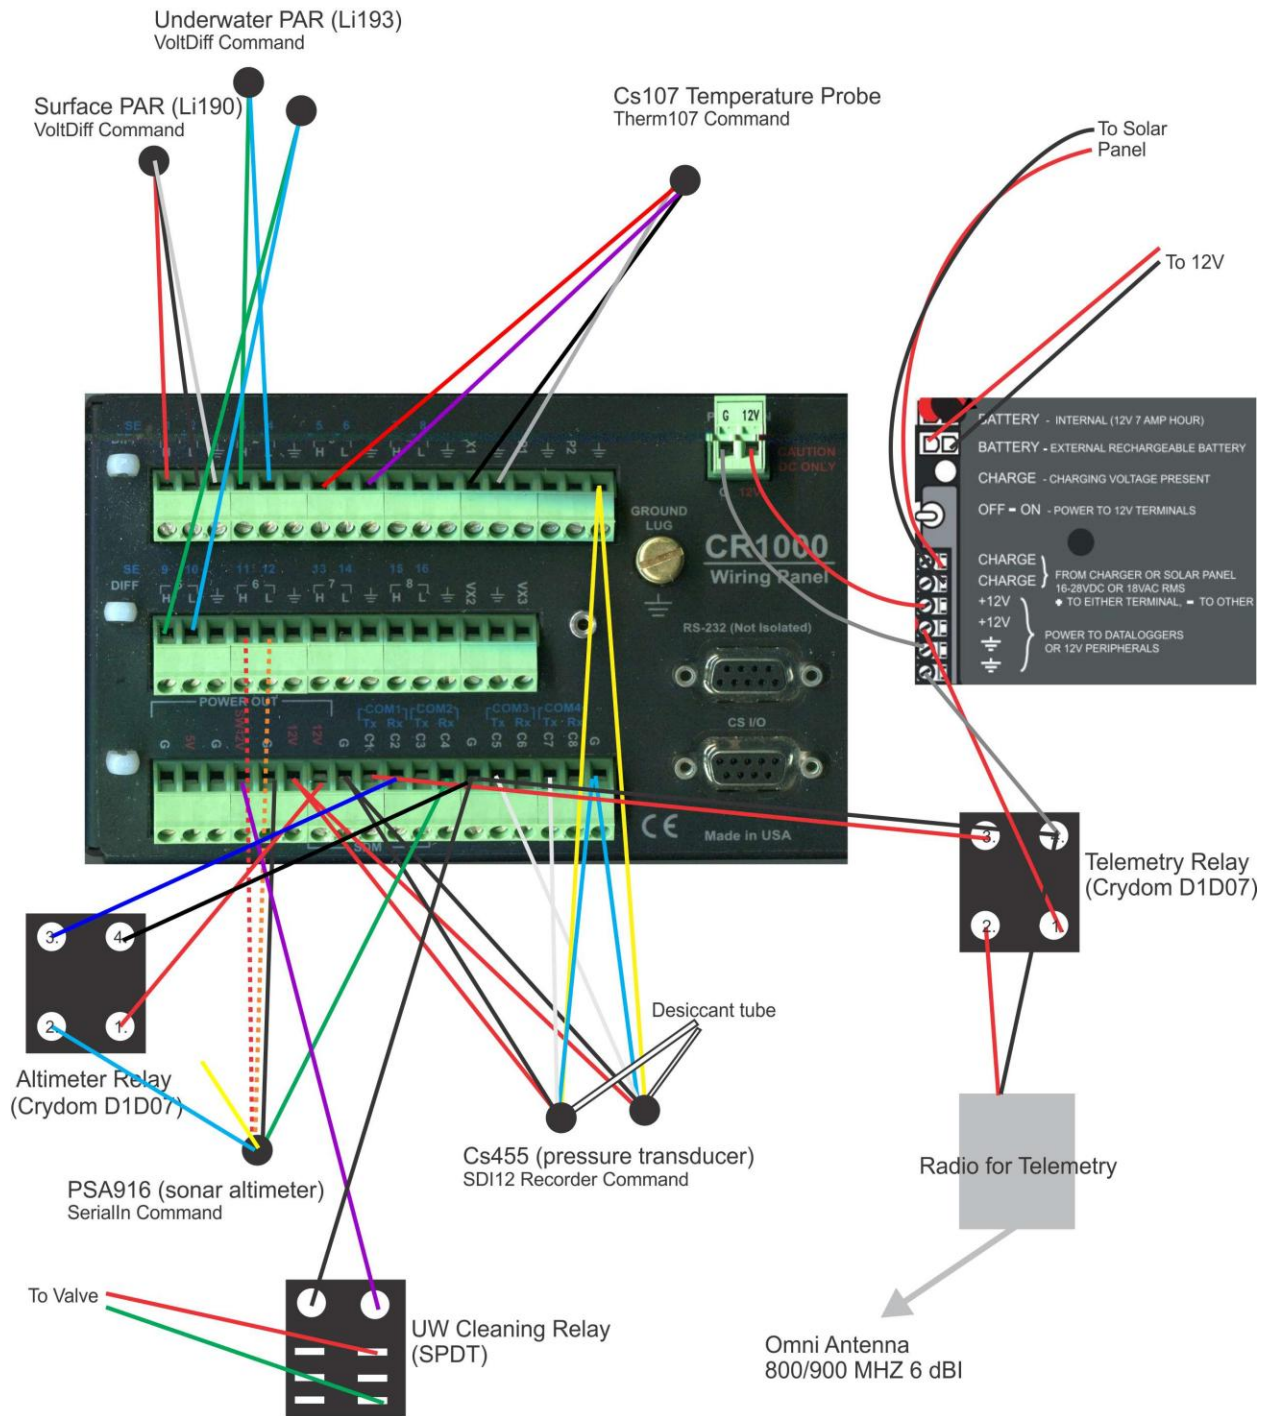

### ***3.1) Fryxell, Hoare, ELB Wiring***

#### **Stage transducer (instrument with desiccant-filled vent tube)**

Red	12V
Black	G
Yellow	G
Blue	G
White	C5
Clear	G

#### **Ablation transducer (instrument with desiccant-filled vent tube)**

Red	12V
Black	G
Yellow	G
Blue	G
White	C7
Clear	G

#### **Underwater PAR\_Moored (diff channel)**

Green	2H
Blue	2L

#### **Underwater PAR\_Hanging (diff channel)**

Green	5H
Blue	5L

#### **Surface PAR (diff channel)**

Red	1H
Black	1L
Silver	G

#### **Sonar Altimeter**

Blue	12v on relay
Black	G
Green	C4
Org/Red	Not used

#### **Temperature Sensor (CS107)**

Black	VX1
Red	SE5
Purple	G
Clear	G

### **3.2) WLB Wiring**

Same as above, except for ablation transducer

#### **Ablation transducer (DRUCK)**

Red	VX2
Black	G
Yellow	8H
Blue	8L
White	G
Orange	not used
Clear	G

### **3.3) Lake Miers Wiring**

**Stage transducer** (instrument with desiccant-filled vent tube)

Red	EX1
Black	3L
Yellow	4H
Blue	4L
White	G
Orange	3H
Clear	G

**Ablation transducer** (instrument with desiccant-filled vent tube)

Red	EX2
Black	5L
Yellow	6H
Blue	6L
White	G
Orange	5H
Clear	G

**Underwater PAR\_Moored (diff channel)**

Green	2H
Blue	2L

**Underwater PAR\_Hanging (diff channel)**

Green	5H
Blue	5L

**Surface PAR (diff channel)**

Black	1L
Red	1H

## 4. Sensor Changes

### 4.1) UNDERWATER PAR sensors. Li-193.

2012/13:

- i) Reset all depths except for Lake Miers
- ii) New bulbs installed on moorings at Lake Hoare, West Lobe Bonney
- iii) A second set of UW PAR sensors was installed at each lake. Cables were hung from the ice.

Lake	S/N	Deployment Date	Deployment Time	Deployed Depth	Calibration date	Multiplier Water	Attachment
Fryxell	SPQA 4628	02/11/2012	18:00	8m		-182.22	Moored
Fryxell	SPQA 4968	15/12/2012	10:20	8m	16/08/2012	-190.81	Hanging
Hoare	SPQA 1694	27/10/2012	18:00	10.1m		-171.92	Moored
Hoare	SPQA 4967	14/12/2012	11:00	10 m	16/08/2012	-187.46	Hanging
ELB	SPQA 4629	14/11/2012		10.06m	24/11/2010	-171.16	Moored
ELB	SPQA 4965	13/12/2012	12:00	10m	16/08/2012	-186.35	Hanging
WLB	SPQA 2870	13/11/2012	18:00	9.86 m	29/06/2012	-196.80	Moored
WLB	SPQA4996	13/12/2012	12:00	10m	16/08/2012	-180.35	Hanging
Miers	SPQA 4630	28/11/2011		9.90m	24/11/2010	-171.36	Moored
Miers	SPQA 4417	18/11/2012	13:30	10m	16/10/2009	-183.53	Hanging

### 4.2) SURFACE PAR sensors. Li-190.

2012/13:

- i) Newly calibrated sensors were replaced at every station

Lake	Season	Deployment Date	S/N	Multiplier ( $\mu\text{m s}^{-1} \text{m}^{-2}$ )
Fryxell	2012/13	02-Nov-12	Q30805	221.3408
Hoare	2012/13	24-Oct-12	Q33694	272.4
ELB	2012/13	14-Nov-12	Q19469	331.7
WLB	2012/13	13-Nov-12	Q20275	238.2
Miers	2011/12	28-Nov-11	Q22174	345.6428

### 4.3) Sonar altimeters. Benthos PSA-916

2012/13:

- i) Sensors were installed at Fryxell, Hoare, ELB and WLB.

Lake	Installation Date	S/N	Depth below water level
<b>Fryxell</b>	02-Nov-12	40138	5.45m
<b>Hoare</b>	22-Oct-12	40266	10.2m
<b>ELB</b>	14-Nov-11	40265	4.52m
<b>WLB</b>	13-Nov-12	?	4.40m

### 4.4) CR1000 Programs

New programs were uploaded at all stations. See section 5.

Note: In the blue box programs, we always have multiplier value of:

- 100 for UW PAR
- 200 for Surface PAR

Real values must be updated in post-processing

Table outputs:

**20min:** Values are measured every 1-min and recorded as 20-min averages.

**15min:** Values are measured every 1-min and recorded as 15-min averages. Begins Jan 1<sup>st</sup>, 2013.

**Minute:** Stage and ablation values are recorded at 1-min intervals.

**Sonar:** Measured at every hour during the summer and every day during the winter.

## 5. CR1000 Programs

### 5.1) Lake Fryxell

'CR1000 Datalogger

'Lake Fryxell

'Sensors installed: Stage, Ablation, UW PAR, surface PAR, surface temp, sonar altimeter

'Additional equipment: UW cleaning system, telemetry radio

'Program written on: Oct 28 2010 by Maciej Obryk

'Program updated on Nov 1, 2012 by Hilary Dugan

'Declare Public Variables

Public PTemp

Public batt\_volt As Float

Public CS455(2) As Float

Public ablation As Float

Public UW\_PAR\_uncorr As Float

Public UW\_PAR\_backup As Float

Public SUR\_PAR\_uncorr As Float

Public MilitaryTime As Float

Public DecTime As Float

Public DecTime\_2 As String \* 16

Public SonarString As String \* 30

Public IceThickness As Float

Public rTime(9) As Float

Public SUR\_Temp As Float

'Declares aliases. rTime = array for Julian time and decimal time

Alias rTime(1) = Year

Alias rTime(4) = Hour

Alias rTime(5) = Minutes

Alias rTime(8) = Day\_of\_Week

Alias rTime(9) = Day\_of\_Year

Alias CS455(1) = stage

Alias CS455(2) = W\_Temp

'Declare Units

Units ablation = m

Units stage = m

Units W\_Temp = degC

Units UW\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$

Units UW\_PAR\_backup =  $\mu\text{mol/s/m}^2$

Units SUR\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$

Units batt\_volt = volts

Units PTemp = degC

Units IceThickness = m

Units SUR\_Temp = degC

'Define Data Tables - what is being stored

DataTable (LF20,true,-1) 'store data points every 20min, averages where indicated below

DataInterval (0,20,Min,10) 'data to storage module; CFM100

CardOut (0,-1)

Sample (1,Year,IEEE4)

```

Sample (1,Day_of_Year,IEEE4)
Sample (1,MilitaryTime,IEEE4)
Sample (1,DecTime,IEEE4)
Sample (1,DecTime_2,String)
Average (1,ablation,IEEE4,False)
Average (1,stage,IEEE4,False)
Average (1,W_Temp,FP2,False)
Average (1,UW_PAR_uncorr,FP2,False)
Average (1,UW_PAR_backup,FP2,False)
Average (1,SUR_PAR_uncorr,IEEE4,False)
Minimum (1,batt_volt,FP2,False,False)'changed to minimum battery voltage
Sample (1,PTemp,FP2)
Average (1,SUR_Temp,FP2,False)

```

EndTable

DataTable (LF15,Year>2012,672) 'store data points every 15min, will start in 2013, only holds one week on internal memory.

```

DataInterval (0,15,Min,10) 'data to storage module; CFM100
CardOut (0,-1)
Sample (1,Year,IEEE4)
Sample (1,Day_of_Year,IEEE4)
Sample (1,MilitaryTime,IEEE4)
Sample (1,DecTime,IEEE4)
Sample (1,DecTime_2,String)
Average (1,ablation,IEEE4,False)
Average (1,stage,IEEE4,False)
Average (1,W_Temp,FP2,False)
Average (1,UW_PAR_uncorr,FP2,False)
Average (1,UW_PAR_backup,FP2,False)
Average (1,SUR_PAR_uncorr,IEEE4,False)
Minimum (1,batt_volt,FP2,False,False)'changed to minimum battery voltage
Sample (1,PTemp,FP2)
Average (1,SUR_Temp,FP2,False)

```

EndTable

DataTable (Sonar,true,-1) 'store sonar altimeter measurements every hour

```

DataInterval (0,1,Hr,10) 'data to storage module; CFM100
CardOut (0,-1)
Average (1,IceThickness,IEEE4,False)

```

EndTable

DataTable (Minute,true,2880) 'store data points every 1min, only holds two days on internal memory.

```

DataInterval (0,1,Min,10) 'data to storage module; CFM100
CardOut (0,-1)
Average (1,ablation,IEEE4,False)
Average (1,stage,IEEE4,False)

```

EndTable

Main Program

BeginProg

```

'measurments every 60 seconds
Scan (60,Sec,1,0)
RealTime (rTime)
MilitaryTime = (Hour*100)+Minutes
'multiplier of "0.704088" is used to covert psi to m, i.e

```



```

'psi to feet = 2.31; feet to m = 0.3048; hence 2.31*0.3048 = 0.704088
SDI12Recorder (ablation,7,0,"M!",0.704088,0) 'pressure transducer - ablation
SDI12Recorder (CS455,5,0,"M!",0.704088,0) 'pressure transducer - stage
'surface PAR - Licor 190
VoltDiff (SUR_PAR_uncorr,1,mV25,1,True ,0,_60Hz,200,0)
'underwater PAR - Licor 193 hanging sensor
VoltDiff (UW_PAR_backup,1,mV2_5,5,True,0,_60Hz,-100,0)
'surface Temperature - CS107 Temperature Probe
Therm107 (SUR_Temp,1,5,Vx1,0,_60Hz,1.0,0)
'datalogger's temp
PanelTemp (PTemp,_60Hz)
'battery voltage
Battery (batt_volt)
'To get high resolution on decimal date, process decimal time in two steps
If (Year/4 - INT(Year/4)) = 0 Then
  DecTime = (Day_of_Year + (Hour + Minutes*(1/60))*(1/24))*(1/367) 'for leap year
Else
  DecTime = (Day_of_Year + (Hour + Minutes*(1/60))*(1/24))*(1/366) 'for normal year
EndIf
DecTime_2 = Year + Replace (DecTime,"0",".")

'underwater PAR - Licor 193
If (Day_of_Year >= 213) OR (Day_of_Year <= 121) Then 'SUMMER
VoltDiff (UW_PAR_uncorr,1,mV2_5,2,True,0,_60Hz,-100,0)
Else,
  UW_PAR_uncorr = "NAN"
EndIf

CallTable LF20
CallTable LF15
CallTable Minute
NextScan

```

SlowSequence 'allows for concurrent sequence scanning

```

Scan (1,Hr,1,0)
If (Day_of_Year >= 274) OR (Day_of_Year <= 60) Then 'SUMMER

  PortSet (2,1)
  Delay(0,3,sec)
  SerialOpen(Com2,9600,0,0,1000) 'UNDERWATER SONAR every hour
  SerialIn (SonarString,Com2,300,13,30)
  'VoltDiff (AnalogOut2,1,mV5000,1,True ,0,_60Hz,1.0,0)
  Delay(0,10,sec)
  SerialClose (Com2)
  PortSet (2,0)
  SplitStr(IceThickness,SonarString,CHR(9),1,0)

  If TimeIntoInterval(0,360,min) Then 'turn on at 0600, 1200,1800,and 0000
  If (batt_volt > 12.4) Then
    PortSet (1,1)
    SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
    Delay (0,2,sec)'delay for Iridium comms
  EndIf
EndIf
If TimeIntoInterval(60,360,min) Then 'turn off at 0700, 1300, 1900, and 0100
  PortSet (1 ,0)

```

```

    SerialClose (ComRS232)
EndIf

If TimeIntoInterval(1,168,hr) Then 'turns on UW PAR cleaning system once a week
    If (batt_volt > 12.4) Then
        SW12(1) 'activates 12V switch port to open SPDT switch
        Delay (0,2,Sec)
        SW12(0) 'closes SPDT switch
    EndIf
EndIf

EndIf

If (Day_of_Year < 274) AND (Day_of_Year > 60) Then 'WINTER
    If TimeIntoInterval(6,24,hr) Then 'turn on once a day at 0600
        If (batt_volt > 12.4) Then 'turn on if above 12V
            PortSet (1,1)
            SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
            Delay (0,2,sec)'delay for Iridium comms
            PortSet (2,1)'UNDERWATER SONAR once a day
            Delay(0,3,sec)
            SerialOpen(Com2,9600,0,0,1000)
            SerialIn (SonarString,Com2,300,13,30)
            Delay(0,10,sec)
            SerialClose (Com2)
            PortSet (2,0)
            SplitStr(IceThickness,SonarString,CHR(9),1,0)
        EndIf
    EndIf
    If TimeIntoInterval(7,24,hr) Then 'turn off at 0700,
        PortSet (1 ,0)
        SerialClose (ComRS232)
        Icethickness = "NAN"
    EndIf

EndIf
CallTable Sonar
NextScan

EndProg

```

## 5.2) Lake Hoare

'CR1000 Datalogger

'Lake Hoare

'Sensors installed: Stage, Ablation, UW PAR, surface PAR, surface temp, sonar altimeter

'Additional equipment: UW cleaning system, telemetry radio

'Program written on: Oct 28 2010 by Maciej Obryk

'Program updated on Dec 14, 2012 by Hilary Dugan

'Declare Public Variables

Public PTemp

Public batt\_volt As Float

Public CS455(2) As Float

Public ablation As Float

Public UW\_PAR\_uncorr As Float

Public UW\_PAR\_backup As Float

Public SUR\_PAR\_uncorr As Float

Public MilitaryTime As Float

Public DecTime As Float

Public DecTime\_2 As String \* 16

Public SonarString As String \* 30

Public IceThickness As Float

Public rTime(9) As Float

Public SUR\_Temp As Float

'Declares aliases. rTime = array for Julian time and decimal time

Alias rTime(1) = Year

Alias rTime(4) = Hour

Alias rTime(5) = Minutes

Alias rTime(8) = Day\_of\_Week

Alias rTime(9) = Day\_of\_Year

Alias CS455(1) = stage

Alias CS455(2) = W\_Temp

'Declare Units

Units ablation = m

Units stage = m

Units W\_Temp = degC

Units UW\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$

Units UW\_PAR\_backup =  $\mu\text{mol/s/m}^2$

Units SUR\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$

Units batt\_volt = volts

Units PTemp = degC

Units IceThickness = m

Units SUR\_Temp = degC

'Define Data Tables - what is being stored

DataTable (LH20,true,-1) 'store data points every 20min, averages where indicated below

DataInterval (0,20,Min,10) 'data to storage module; CFM100

CardOut (0,-1)

Sample (1,Year,IEEE4)

Sample (1,Day\_of\_Year,IEEE4)

Sample (1,MilitaryTime,IEEE4)

Sample (1,DecTime,IEEE4)

Sample (1,DecTime\_2,String)

Average (1,ablation,IEEE4,False)

```

Average (1,stage,IEEE4,False)
Average (1,W_Temp,FP2,False)
Average (1,UW_PAR_uncorr,FP2,False)
Average (1,UW_PAR_backup,FP2,False)
Average (1,SUR_PAR_uncorr,IEEE4,False)
Minimum (1,batt_volt,FP2,False,False)'changed to minimum battery voltage
Sample (1,PTemp,FP2)
Average (1,SUR_Temp,FP2,False)

```

EndTable

DataTable (LH15,Year>2012,672) 'store data points every 15min, will start in 2013, only holds one week on internal memory.

```

DataInterval (0,15,Min,10) 'data to storage module; CFM100
CardOut (0,-1)
Sample (1,Year,IEEE4)
Sample (1,Day_of_Year,IEEE4)
Sample (1,MilitaryTime,IEEE4)
Sample (1,DecTime,IEEE4)
Sample (1,DecTime_2,String)
Average (1,ablation,IEEE4,False)
Average (1,stage,IEEE4,False)
Average (1,W_Temp,FP2,False)
Average (1,UW_PAR_uncorr,FP2,False)
Average (1,UW_PAR_backup,FP2,False)
Average (1,SUR_PAR_uncorr,IEEE4,False)
Minimum (1,batt_volt,FP2,False,False)'changed to minimum battery voltage
Sample (1,PTemp,FP2)
Average (1,SUR_Temp,FP2,False)
EndTable

```

DataTable (Sonar,true,-1) 'store sonar altimeter measurements every hour

```

DataInterval (0,1,Hr,10) 'data to storage module; CFM100
CardOut (0,-1)
Average (1,IceThickness,IEEE4,False)
EndTable

```

DataTable (Minute,true,2880) 'store data points every 1min, only holds two days on internal memory.

```

DataInterval (0,1,Min,10) 'data to storage module; CFM100
CardOut (0,-1)
Average (1,ablation,IEEE4,False)
Average (1,stage,IEEE4,False)
EndTable

```

'Main Program

BeginProg

```

'measurments every 60 seconds
Scan (60,Sec,1,0)
RealTime (rTime)
MilitaryTime = (Hour*100)+Minutes
'multiplier of "0.704088" is used to covert psi to m, i.e
'psi to feet = 2.31; feet to m = 0.3048; hence 2.31*0.3048 = 0.704088
SDI12Recorder (ablation,7,0,"M!",0.704088,0) 'pressure transducer - ablation
SDI12Recorder (CS455,5,0,"M!",0.704088,0) 'pressure transducer - stage
'surface PAR - Licor 190
VoltDiff (SUR_PAR_uncorr,1,mV25,1,True ,0,_60Hz,200,0)

```

```

'underwater PAR - Licor 193 hanging sensor
VoltDiff (UW_PAR_backup,1,mV2_5,5,True,0,_60Hz,-100,0)
'surface Temperature - CS107 Temperature Probe
Therm107 (SUR_Temp,1,5,Vx1,0,_60Hz,1.0,0)
'datalogger's temp
PanelTemp (PTemp,_60Hz)
'battery voltage
Battery (batt_volt)
'To get high resolution on decimal date, process decimal time in two steps
If (Year/4 - INT(Year/4)) = 0 Then
  DecTime = (Day_of_Year + (Hour + Minutes*(1/60))*(1/24))*(1/367) 'for leap year
Else
  DecTime = (Day_of_Year + (Hour + Minutes*(1/60))*(1/24))*(1/366) 'for normal year
EndIf
DecTime_2 = Year + Replace (DecTime,"0.",".")

```

```

'underwater PAR - Licor 193
If (Day_of_Year >= 213) OR (Day_of_Year <= 121) Then 'SUMMER
VoltDiff (UW_PAR_uncorr,1,mV2_5,2,True,0,_60Hz,-100,0)
Else,
  UW_PAR_uncorr = "NAN"
EndIf

```

```

CallTable LH20
CallTable LH15
CallTable Minute
NextScan

```

SlowSequence 'allows for concurrent sequence scanning

```

Scan (1,Hr,1,0)
If (Day_of_Year >= 274) OR (Day_of_Year <= 60) Then 'SUMMER

```

```

  PortSet (2,1)
  Delay(0,3,sec)
  SerialOpen(Com2,9600,0,0,1000) 'UNDERWATER SONAR every hour
  SerialIn (SonarString,Com2,300,13,30)
  'VoltDiff (AnalogOut2,1,mV5000,1,True ,0,_60Hz,1.0,0)
  Delay(0,10,sec)
  SerialClose (Com2)
  PortSet (2,0)
  SplitStr(IceThickness,SonarString,CHR(9),1,0)

```

```

If TimeIntoInterval(60,360,min) Then 'turn on at 0700, 1300, 1900, and 0100

```

```

  If (batt_volt > 12.4) Then
    PortSet (1,1)
    SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
    Delay (0,2,sec)'delay for Iridium comms
  EndIf

```

```

EndIf
If TimeIntoInterval(120,360,min) Then 'turn off at 0800, 1400, 2000, and 0200

```

```

  PortSet (1 ,0)
  SerialClose (ComRS232)

```

```

EndIf

```

```

If TimeIntoInterval(1,168,hr) Then 'turns on UW PAR cleaning system once a week

```

```

  If (batt_volt > 12.4) Then

```

```

    SW12(1) 'activates 12V switch port to open SPDT switch
    Delay (0,2,Sec)
    SW12(0) 'closes SPDT switch
    EndIf
EndIf

EndIf

If (Day_of_Year < 274) AND (Day_of_Year > 60) Then 'WINTER
If TimeIntoInterval(7,24,hr) Then 'turn on once a day at 0700
If (batt_volt > 12.4) Then 'turn on if above 12V
    PortSet (1,1)
    SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
    Delay (0,2,sec)'delay for Iridium comms
    PortSet (2,1)'UNDERWATER SONAR once a day
    Delay(0,3,sec)
    SerialOpen(Com2,9600,0,0,1000)
    SerialIn (SonarString,Com2,300,13,30)
    Delay(0,10,sec)
    SerialClose (Com2)
    PortSet (2,0)
    SplitStr(IceThickness,SonarString,CHR(9),1,0)
EndIf
EndIf
If TimeIntoInterval(8,24,hr) Then 'turn off at 0800,
    PortSet (1 ,0)
    SerialClose (ComRS232)
    Icethickness = "NAN"
EndIf

EndIf
CallTable Sonar
NextScan

EndProg

```

### 5.3) East Lake Bonney

'CR1000 Datalogger  
'East Lake Bonney  
'Sensors installed: Stage, Ablation, UW PAR, surface PAR, surface temp, sonar altimeter  
'Additional equipment: UW cleaning system, telemetry radio  
'Program written on: Oct 28 2010 by Maciej Obryk  
'Program updated on Nov 15, 2012 by Hilary Dugan

'Declare Public Variables  
Public PTemp  
Public batt\_volt As Float  
Public CS455(2) As Float  
Public ablation As Float  
Public UW\_PAR\_uncorr As Float  
Public UW\_PAR\_backup As Float  
Public SUR\_PAR\_uncorr As Float  
Public MilitaryTime As Float  
Public DecTime As Float  
Public DecTime\_2 As String \* 16  
Public SonarString As String \* 30  
Public IceThickness As Float  
Public rTime(9) As Float  
Public SUR\_Temp As Float

'Declares aliases. rTime = array for Julian time and decimal time  
Alias rTime(1) = Year  
Alias rTime(4) = Hour  
Alias rTime(5) = Minutes  
Alias rTime(8) = Day\_of\_Week  
Alias rTime(9) = Day\_of\_Year  
Alias CS455(1) = stage  
Alias CS455(2) = W\_Temp

'Declare Units  
Units ablation = m  
Units stage = m  
Units W\_Temp = degC  
Units UW\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$   
Units UW\_PAR\_backup =  $\mu\text{mol/s/m}^2$   
Units SUR\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$   
Units batt\_volt = volts  
Units PTemp = degC  
Units IceThickness = m  
Units SUR\_Temp = degC

'Define Data Tables - what is being stored  
DataTable (ELB20,true,-1) 'store data points every 20min, averages where indicated below  
DataInterval (0,20,Min,10) 'data to storage module; CFM100  
CardOut (0,-1)  
Sample (1,Year,IEEE4)  
Sample (1,Day\_of\_Year,IEEE4)  
Sample (1,MilitaryTime,IEEE4)  
Sample (1,DecTime,IEEE4)  
Sample (1,DecTime\_2,String)  
Average (1,ablation,IEEE4,False)

```

Average (1,stage,IEEE4,False)
Average (1,W_Temp,FP2,False)
Average (1,UW_PAR_uncorr,FP2,False)
Average (1,UW_PAR_backup,FP2,False)
Average (1,SUR_PAR_uncorr,IEEE4,False)
Minimum (1,batt_volt,FP2,False,False)'changed to minimum battery voltage
Sample (1,PTemp,FP2)
Average (1,SUR_Temp,FP2,False)

```

EndTable

DataTable (ELB15,Year>2012,672) 'store data points every 15min, will start in 2013, only holds one week on internal memory.

```

DataInterval (0,15,Min,10) 'data to storage module; CFM100
CardOut (0,-1)
Sample (1,Year,IEEE4)
Sample (1,Day_of_Year,IEEE4)
Sample (1,MilitaryTime,IEEE4)
Sample (1,DecTime,IEEE4)
Sample (1,DecTime_2,String)
Average (1,ablation,IEEE4,False)
Average (1,stage,IEEE4,False)
Average (1,W_Temp,FP2,False)
Average (1,UW_PAR_uncorr,FP2,False)
Average (1,UW_PAR_backup,FP2,False)
Average (1,SUR_PAR_uncorr,IEEE4,False)
Minimum (1,batt_volt,FP2,False,False)'changed to minimum battery voltage
Sample (1,PTemp,FP2)
Average (1,SUR_Temp,FP2,False)
EndTable

```

DataTable (Sonar,true,-1) 'store sonar altimeter measurements every hour

```

DataInterval (0,1,Hr,10) 'data to storage module; CFM100
CardOut (0,-1)
Average (1,IceThickness,IEEE4,False)
EndTable

```

DataTable (Minute,true,2880) 'store data points every 1min, only holds two days on internal memory.

```

DataInterval (0,1,Min,10) 'data to storage module; CFM100
CardOut (0,-1)
Average (1,ablation,IEEE4,False)
Average (1,stage,IEEE4,False)
EndTable

```

'Main Program

BeginProg

```

'measurments every 60 seconds
Scan (60,Sec,1,0)
RealTime (rTime)
MilitaryTime = (Hour*100)+Minutes
'multiplier of "0.704088" is used to covert psi to m, i.e
'psi to feet = 2.31; feet to m = 0.3048; hence 2.31*0.3048 = 0.704088
SDI12Recorder (ablation,7,0,"M!",0.704088,0) 'pressure transducer - ablation
SDI12Recorder (CS455,5,0,"M!",0.704088,0) 'pressure transducer - stage
'surface PAR - Licor 190
VoltDiff (SUR_PAR_uncorr,1,mV25,1,True ,0,_60Hz,200,0)

```



```

'underwater PAR - Licor 193 hanging sensor
VoltDiff (UW_PAR_backup,1,mV2_5,5,True,0,_60Hz,-100,0)
'surface Temperature - CS107 Temperature Probe
Therm107 (SUR_Temp,1,5,Vx1,0,_60Hz,1.0,0)
'datalogger's temp
PanelTemp (PTemp,_60Hz)
'batttry voltage
Battery (batt_volt)
'To get high resolution on decimal date, process decimal time in two steps
If (Year/4 - INT(Year/4)) = 0 Then
  DecTime = (Day_of_Year + (Hour + Minutes*(1/60))*(1/24))*(1/367) 'for leap year
Else
  DecTime = (Day_of_Year + (Hour + Minutes*(1/60))*(1/24))*(1/366) 'for normal year
EndIf
DecTime_2 = Year + Replace (DecTime,"0.",".")

```

```

'underwater PAR - Licor 193
If (Day_of_Year >= 213) OR (Day_of_Year <= 121) Then 'SUMMER
VoltDiff (UW_PAR_uncorr,1,mV2_5,2,True,0,_60Hz,-100,0)
Else,
  UW_PAR_uncorr = "NAN"
EndIf

```

```

CallTable ELB20
CallTable ELB15
CallTable Minute
NextScan

```

SlowSequence 'allows for concurrent sequence scanning

```

Scan (1,Hr,1,0)
If (Day_of_Year >= 274) OR (Day_of_Year <= 60) Then 'SUMMER

```

```

  PortSet (2,1)
  Delay(0,3,sec)
  SerialOpen(Com2,9600,0,0,1000) 'UNDERWATER SONAR every hour
  SerialIn (SonarString,Com2,300,13,30)
  'VoltDiff (AnalogOut2,1,mV5000,1,True ,0,_60Hz,1.0,0)
  Delay(0,10,sec)
  SerialClose (Com2)
  PortSet (2,0)
  SplitStr(IceThickness,SonarString,CHR(9),1,0)

```

```

If TimeIntoInterval(60,360,min) Then 'turn on at 0700, 1300, 1900, and 0100

```

```

  If (batt_volt > 12.4) Then
    PortSet (1,1)
    SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
    Delay (0,2,sec)'delay for Iridium comms
  EndIf

```

```

EndIf
If TimeIntoInterval(120,360,min) Then 'turn off at 0800, 1400, 2000, and 0200

```

```

  PortSet (1 ,0)
  SerialClose (ComRS232)

```

```

EndIf

```

```

If TimeIntoInterval(1,168,hr) Then 'turns on UW PAR cleaning system once a week

```

```

  If (batt_volt > 12.4) Then

```

```

    SW12(1) 'activates 12V switch port to open SPDT switch
    Delay (0,2,Sec)
    SW12(0) 'closes SPDT switch
  EndIf
EndIf

EndIf

If (Day_of_Year < 274) AND (Day_of_Year > 60) Then 'WINTER
  If TimeIntoInterval(7,24,hr) Then 'turn on once a day at 0700
    If (batt_volt > 12.4) Then 'turn on if above 12V
      PortSet (1,1)
      SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
      Delay (0,2,sec)'delay for Iridium comms
      PortSet (2,1)'UNDERWATER SONAR once a day
      Delay(0,3,sec)
      SerialOpen(Com2,9600,0,0,1000)
      SerialIn (SonarString,Com2,300,13,30)
      Delay(0,10,sec)
      SerialClose (Com2)
      PortSet (2,0)
      SplitStr(IceThickness,SonarString,CHR(9),1,0)
    EndIf
  EndIf
  If TimeIntoInterval(8,24,hr) Then 'turn off at 0800,
    PortSet (1 ,0)
    SerialClose (ComRS232)
    Icethickness = "NAN"
  EndIf

  EndIf
  CallTable Sonar
NextScan

EndProg

```

## 5.4) West Lake Bonney

'CR1000 Datalogger

'West Lobe Bonney

'Sensors installed: Stage, Ablation, UW PAR, surface PAR, surface temp, sonar altimeter

'Additional equipment: UW cleaning system, telemetry radio

'Program written on: Oct 28 2010 by Maciej Obryk

'Program updated on Nov 8, 2012 by Hilary Dugan

'Declare Public Variables

Public PTemp

Public batt\_volt As Float

Public CS455(2) As Float

Public ablation As Float

Public UW\_PAR\_uncorr As Float

Public UW\_PAR\_backup As Float

Public SUR\_PAR\_uncorr As Float

Public MilitaryTime As Float

Public DecTime As Float

Public DecTime\_2 As String \* 16

Public SonarString As String \* 30

Public IceThickness As Float

Public rTime(9) As Float

Public SUR\_Temp As Float

'Declares aliases. rTime = array for Julian time and decimal time

Alias rTime(1) = Year

Alias rTime(4) = Hour

Alias rTime(5) = Minutes

Alias rTime(8) = Day\_of\_Week

Alias rTime(9) = Day\_of\_Year

Alias CS455(1) = stage

Alias CS455(2) = W\_Temp

'Declare Units

Units ablation = m

Units stage = m

Units W\_Temp = degC

Units UW\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$

Units UW\_PAR\_backup =  $\mu\text{mol/s/m}^2$

Units SUR\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$

Units batt\_volt = volts

Units PTemp = degC

Units IceThickness = m

Units SUR\_Temp = degC

'Define Data Tables - what is being stored

DataTable (WLB20,true,-1) 'store data points every 20min, averages where indicated below

DataInterval (0,20,Min,10) 'data to storage module; CFM100

CardOut (0,-1)

Sample (1,Year,IEEE4)

Sample (1,Day\_of\_Year,IEEE4)

Sample (1,MilitaryTime,IEEE4)

Sample (1,DecTime,IEEE4)

Sample (1,DecTime\_2,String)

```

Average (1,ablation,IIEEE4,False)
Average (1,stage,IIEEE4,False)
Average (1,W_Temp,FP2,False)
Average (1,UW_PAR_uncorr,FP2,False)
Average (1,UW_PAR_backup,FP2,False)
Average (1,SUR_PAR_uncorr,IIEEE4,False)
Minimum (1,batt_volt,FP2,False,False)'changed to minimum battery voltage
Sample (1,PTemp,FP2)
Average (1,SUR_Temp,FP2,False)

```

EndTable

DataTable (WLB15,Year>2012,672) 'store data points every 15min, will start in 2013, only holds one week on internal memory.

```

DataInterval (0,15,Min,10) 'data to storage module; CFM100
CardOut (0,-1)
Sample (1,Year,IIEEE4)
Sample (1,Day_of_Year,IIEEE4)
Sample (1,MilitaryTime,IIEEE4)
Sample (1,DecTime,IIEEE4)
Sample (1,DecTime_2,String)
Average (1,ablation,IIEEE4,False)
Average (1,stage,IIEEE4,False)
Average (1,W_Temp,FP2,False)
Average (1,UW_PAR_uncorr,FP2,False)
Average (1,UW_PAR_backup,FP2,False)
Average (1,SUR_PAR_uncorr,IIEEE4,False)
Minimum (1,batt_volt,FP2,False,False)'changed to minimum battery voltage
Sample (1,PTemp,FP2)
Average (1,SUR_Temp,FP2,False)

```

EndTable

DataTable (Sonar,true,-1) 'store sonar altimeter measurements every hour

```

DataInterval (0,1,Hr,10) 'data to storage module; CFM100
CardOut (0,-1)
Average (1,IceThickness,IIEEE4,False)

```

EndTable

DataTable (Minute,true,2880) 'store data points every 1min, only holds two days on internal memory.

```

DataInterval (0,1,Min,10) 'data to storage module; CFM100
CardOut (0,-1)
Average (1,ablation,IIEEE4,False)
Average (1,stage,IIEEE4,False)

```

EndTable

'Main Program

BeginProg

```

'measurments every 60 seconds
Scan (60,Sec,1,0)
RealTime (rTime)
MilitaryTime = (Hour*100)+Minutes
'multiplier of "0.704088" is used to covert psi to m, i.e
'psi to feet = 2.31; feet to m = 0.3048; hence 2.31*0.3048 = 0.704088
SDI12Recorder (CS455,5,0,"M!",0.704088,0) 'pressure transducer - stage
'CS420/CS425 Druck PDCR 1830/1230 Pressure Tansducer (4-wire) measurement Lvl_m:

```

```

BrFull(ablation,1,mV2500,8,Vx2,1,2500,True,True,0,_60Hz,101.53,0.0)
'surface PAR - Licor 190
VoltDiff (SUR_PAR_uncorr,1,mV25,1,True ,0,_60Hz,200,0)
'underwater PAR - Licor 193 hanging sensor
VoltDiff (UW_PAR_backup,1,mV2_5,5,True,0,_60Hz,-100,0)
'surface Temperature - CS107 Temperature Probe
Therm107 (SUR_Temp,1,5,Vx1,0,_60Hz,1.0,0)
'datalogger's temp
PanelTemp (PTemp,_60Hz)
'battery voltage
Battery (batt_volt)
'To get high resolution on decimal date, process decimal time in two steps
If (Year/4 - INT(Year/4)) = 0 Then
  DecTime = (Day_of_Year + (Hour + Minutes*(1/60))*(1/24))*(1/367) 'for leap year
Else
  DecTime = (Day_of_Year + (Hour + Minutes*(1/60))*(1/24))*(1/366) 'for normal year
EndIf
DecTime_2 = Year + Replace (DecTime,"0.",".")

'underwater PAR - Licor 193
If (Day_of_Year >= 213) OR (Day_of_Year <= 121) Then 'SUMMER
VoltDiff (UW_PAR_uncorr,1,mV2_5,2,True,0,_60Hz,-100,0)
Else,
  UW_PAR_uncorr = "NAN"
EndIf

CallTable WLB20
CallTable WLB15
CallTable Minute
NextScan

```

SlowSequence 'allows for concurrent sequence scanning

```

Scan (1,Hr,1,0)
If (Day_of_Year >= 274) OR (Day_of_Year <= 60) Then 'SUMMER

  PortSet (2,1)
  Delay(0,3,sec)
  SerialOpen(Com2,9600,0,0,1000) 'UNDERWATER SONAR every hour
  SerialIn (SonarString,Com2,300,13,30)
  'VoltDiff (AnalogOut2,1,mV5000,1,True ,0,_60Hz,1.0,0)
  Delay(0,10,sec)
  SerialClose (Com2)
  PortSet (2,0)
  SplitStr(IceThickness,SonarString,CHR(9),1,0)

  If TimeIntoInterval(0,360,min) Then 'turn on at 0600, 1200,1800,and 0000
    If (batt_volt > 12.4) Then
      PortSet (1,1)
      SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
      Delay (0,2,sec)'delay for Iridium comms
    EndIf
  EndIf

  If TimeIntoInterval(60,360,min) Then 'turn off at 0700, 1300, 1900, and 0100
    PortSet (1 ,0)
    SerialClose (ComRS232)
  EndIf

```

```

If TimeIntoInterval(1,168,hr) Then 'turns on UW PAR cleaning system once a week
  If (batt_volt > 12.4) Then
    SW12(1) 'activates 12V switch port to open SPDT switch
    Delay (0,2,Sec)
    SW12(0) 'closes SPDT switch
  EndIf
EndIf

EndIf

If (Day_of_Year < 274) AND (Day_of_Year > 60) Then 'WINTER
  If TimeIntoInterval(6,24,hr) Then 'turn on once a day at 0600
    If (batt_volt > 12.4) Then 'turn on if above 12V
      PortSet (1,1)
      SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
      Delay (0,2,sec)'delay for Iridium comms
      PortSet (2,1)'UNDERWATER SONAR once a day
      Delay(0,3,sec)
      SerialOpen(Com2,9600,0,0,1000)
      SerialIn (SonarString,Com2,300,13,30)
      Delay(0,10,sec)
      SerialClose (Com2)
      PortSet (2,0)
      SplitStr(IceThickness,SonarString,CHR(9),1,0)
    EndIf
  EndIf
  If TimeIntoInterval(7,24,hr) Then 'turn off at 0700,
    PortSet (1 ,0)
    SerialClose (ComRS232)
    Icethickness = "NAN"
  EndIf

  EndIf
  CallTable Sonar
NextScan

EndProg

```

## 5.5) Lake Miers

'CR1000 Datalogger

'Lake Miers

'Sensors installed: Stage, Ablation, UW PAR, surface PAR

'Program written on: Nov 15 2011 by Maciej Obryk

'Updated on Nov 15, 2012 by Hilary Dugan

'Declare Variables

Public batt\_volt As Float

Public stage As Float

Public ablation As Float

Public UW\_PAR\_uncorr As Float

Public UW\_PAR\_backup As Float

Public surface\_PAR\_uncorr As Float

Public Ptemp\_C

Public flag As Boolean

'Declares array for Julian time and decimal time

Public rTime (9)

Alias rTime(1) = Year

Alias rTime(8) = Day\_of\_Week

Alias rTime(9) = Day\_of\_Year

Alias rtime(4) = Hour

Alias rtime(5) = Minutes

Public Dec\_Time As Float

Public MilitaryTime As Float

Public DecTime As Float

Public DecTime\_2 As String \* 16

'Declares Units

Units batt\_volt = volts

Units UW\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$

Units UW\_PAR\_backup =  $\mu\text{mol/s/m}^2$

Units surface\_PAR\_uncorr =  $\mu\text{mol/s/m}^2$

Units stage = cm

Units ablation = cm

Units PTemp\_C = Deg C

'Defines Data Tables

DataTable(LM20,True,-1)

'store data points every 20min

DataInterval(0,20,Min,10)

CardOut (0 ,-1)

Sample (1,Year,IIEEE4)

Sample (1,Day\_of\_Year,IIEEE4)

Sample (1,MilitaryTime,IIEEE4)

Sample (1,DecTime,IIEEE4)

Sample (1,DecTime\_2,String)

Average(1,stage,IIEEE4,False)

Average(1,ablation,IIEEE4,False)

Average(1,UW\_PAR\_uncorr,IIEEE4,False)

Average(1,UW\_PAR\_backup,IIEEE4,False)

Average(1,surface\_PAR\_uncorr,IIEEE4,False)

Average(1,batt\_volt,FP2,False)

Average(1,Ptemp\_C,FP2, False)

EndTable

DataTable(LM15,Year>2012,672) 'store data points every 15min, will start in 2013, only holds one week on internal memory.

```
'store data points every 20min
DataInterval(0,15,Min,10)
CardOut (0,-1)
Sample (1,Year,IEEE4)
Sample (1,Day_of_Year,IEEE4)
Sample (1,MilitaryTime,IEEE4)
Sample (1,DecTime,IEEE4)
Sample (1,DecTime_2,String)
Average(1,stage,IEEE4,False)
Average(1,ablation,IEEE4,False)
Average(1,UW_PAR_uncorr,IEEE4,False)
Average(1,UW_PAR_backup,IEEE4,False)
Average(1,surface_PAR_uncorr,IEEE4,False)
Average(1,batt_volt,FP2,False)
Average(1,Ptemp_C,FP2, False)
```

EndTable

Main Program

BeginProg

```
Scan(60,Sec,1,0)
RealTime rTime()
MilitaryTime = (Hour*100)+Minutes
'surface PAR - Licor 190
VoltDiff(surface_PAR_uncorr,1,mV25,1,True,0,_60Hz,200,0)
'underwater PAR - Licor 193
VoltDiff(UW_PAR_backup,1,mV2_5,8,True,0,_60Hz,-100,0)
'CS420/CS425 Druck PDCR 1830/1230 Pressure Tansducer (6-wire) measurement:
BrFull6W (stage,1,mV2500,mV25,3,Vx1,1,2500,True ,True ,0,_60Hz,1.0,0)
BrFull6W (ablation,1,mV2500,mV25,5,Vx2,1,2500,True ,True ,0,_60Hz,1.0,0)
PanelTemp (Ptemp_C,_60Hz)
Battery (batt_volt)
```

'underwater PAR - Licor 193

If (Day\_of\_Year >= 213) OR (Day\_of\_Year <= 121) Then 'SUMMER

VoltDiff(UW\_PAR\_uncorr,1,mV2\_5,2,True,0,\_60Hz,-100,0)

Else,

UW\_PAR\_uncorr = "NAN"

EndIf

"To get high resolution on decimal date, process decimal time in two steps

If (Year/4 - INT(Year/4)) = 0 Then

DecTime = (Day\_of\_Year + (Hour + Minutes\*(1/60))\*(1/24))\*(1/367) 'for leap year

Else

DecTime = (Day\_of\_Year + (Hour + Minutes\*(1/60))\*(1/24))\*(1/366) 'for normal year

EndIf

DecTime\_2 = Year + Replace (DecTime,"0.",".")

CallTable LM20

CallTable LM15

NextScan

SlowSequence 'allows for concurrent sequence scanning



```

Scan (1,Hr,1,0)
If (Day_of_Year >= 274) OR (Day_of_Year <= 60) Then 'SUMMER
  If TimeIntoInterval(180,360,min) Then 'turn on at 0900, 1500, 2100 and 0300
    If (batt_volt > 12.4) Then
      PortSet (1,1)
      SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
      Delay (0,2,sec)'delay for Iridium comms
    EndIf
  EndIf
  If TimeIntoInterval(240,360,Min) Then 'turn off ComRS232 at 1000, 1600, 2200 and 0400
    PortSet (1 ,0)
    SerialClose (ComRS232)
  EndIf
EndIf

If (Day_of_Year < 274) AND (Day_of_Year > 60) Then 'WINTER
  If TimeIntoInterval(9,24,hr) Then 'turn on once a day at 0900
    If (batt_volt > 12.4) Then 'turn on if above 12V
      PortSet (1,1)
      SerialOpen (ComRS232,9600,0,0,2000) 'enables CR1000 comms
      Delay (0,2,sec)'delay for Iridium comms
    EndIf
  EndIf
  If TimeIntoInterval(10,24,hr) Then 'turn off at 1000,
    PortSet (1,0)
    SerialClose (ComRS232)
  EndIf
EndIf
NextScan

EndProg

```